

EMR Timeline Lab Tooltip Display Company Setting

Last Modified on 03/21/2024 1:35 pm EDT



Currently, when users access the EMR and view the Patient's Timeline, the Lab icon tool-tip displays the short description for the first 5 lab orders when you hover over the Lab icon. The user has no idea if other lab tests were run and resulted, or if what they are seeing is everything. In Release 24.105 we have added new Company Setting that will allow users to deviate from this default.

Available for Beta currently - expected for full production in a 2024 Q2 release

EMR Timeline Hover Text Updates available for clients using the (Beta) New EMR Timeline

In the New EMR Timeline when users hover over the Lab icon, the tool-tip will continue to display the first five short lab short description names as a default. However, users will notice that when there are other labs not displayed, they will see an ellipsis displayed as an indicator to the user that there are more lab tests that what is listed.

If a practice wants to adjust the default of displaying five lab text names to more or less, they can use the new company setting (noted below).

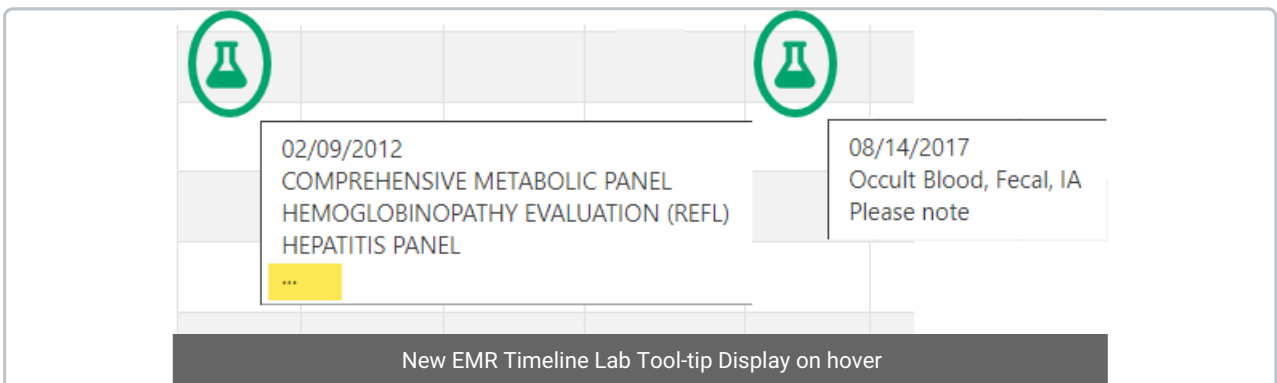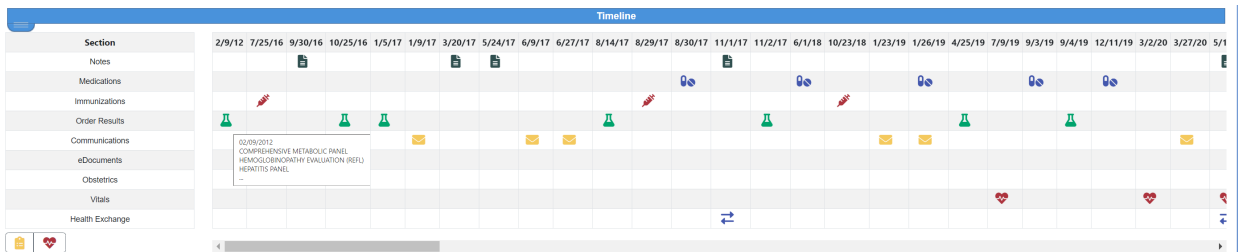

Company Setting

If your practice wants to display more than the default 5 tool-tip displays (lab short descriptions) when you hover over the Lab icon, then you will need practice users with the ability to access Company Settings would need to set the Company Setting: Timeline orders hover maximum display limit setting and designate their desired display. This link takes you to the Knowledge Owl articles for everything you need to know about Company Settings. The maximum that can be set to display is 100.

The screenshot shows the EMR interface for a patient named 'Imbes, Beverly A.'. The main window displays the patient's chart with sections for Allergies, Medications, and Problems. A 'Vitals Timeline' window is open, showing a grid of vital signs (C, H, P, W, R, T, S, O, SpO2, BP, HR, RR, Temp) over time. A 'Company Setting' dialog box is overlaid on the timeline, showing the 'Timeline orders hover maximum display limit' setting set to 3. The dialog also includes a search bar and a 'Company Setting' section with a description of the setting.

Company Setting: Timeline orders hover maximum display limit
 This setting can be found in the Company Settings window under Reporting-EMR Settings. This setting is set to '22' for the practice. Set the maximum number of orders to display on hover for a specific date.

Company Setting: Wireframe List for Vitals Timeline Wireframe Summary
 This setting can be found in the Company Settings window under Reporting-EMR Settings. This setting is set to 'Dev Ops, Health, CBC, Diabetes, Lipid, PSA, Triglyceride, Test' for the practice. Comma delimited list of wireframes that will be displayed when the user selects a vitals entry on the EMR timeline screen for a patient. Valid entries are pulled from the Fish Bone List descriptors within the admin/Fish Bone screen. Default value is 'CBC'.